



PORTABLE INSTRUMENTS

SOFTWARE


ACCESSORIES

ALARM / PROTECTION, LEVEL

DAKKS CALIBRATION CERTIFICATE

DAKKS calibration certificates are used for very high-quality calibrations and calibrate reference instruments or standards and regulations requiring those certificates. DAKKS-DKD calibration certificates are issued using reference instruments for which traceability is ensured through a link to the laboratory of the Physikalische Bundesanstalt. DAKKS-DKD calibration certificates can only be issued by calibration laboratories accredited according to the DIN EN ISO 17025 standard.

Periodic external assessment and reaccreditation ensure that calibration is of a consistently high quality. These costs- and personnel-intensive measures result in a higher price, but, in return, provide the necessary reliability in the measurement results. Successful DAKKS assessment of the Greisinger site for the measured variable temperature. The calibration laboratory has been working in accordance with DIN EN ISO / IEC 17025 since 2018.

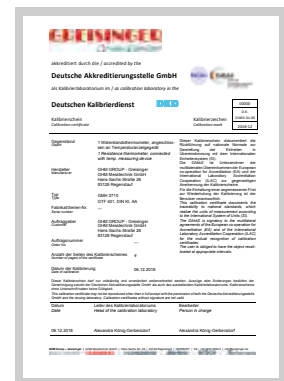

TEMPERATURE

DAKKS-T
 Calibration certificate temperature, including 1 test point (please always specify the test point)

additional test points
 (from -100 .. + 1400 °C) please always specify test point)

additional test points
 -196 °C

THE ACCREDITATION IS ONLY VALID FOR THE SCOPE OF ACCREDITATION LISTED IN THE DOCUMENT DK-21043-01-00.

Deutsche Akkreditierungsstelle
 D-K-21043-01-00

PRESSURE

DAKKS-P
 Item No. 602731
 DAKKS calibration certificate overpressure -1..100 bar (pressure, 9 test points rising and falling, procedure B, target: 0.1..0.6 % measuring span)

DAKKS-PA
 Item No. 602758
 DAKKS calibration certificate absolute pressure 0..70 bar (absolute pressure, 9 test points rising and falling, Sequence B, Target: 0.1..0.6 % measuring span)

further measuring ranges and accuracies on request

HUMIDITY (INCL. 1 TEMPERATURE VALUE)

DAKKS-FE
 Item No. 602871
 DAKKS calibration certificate, humidity (device with external sensor); (test points: humidity 15 %, 70 % and temperature approx. 23 °C)

DAKKS-F
 Item No. 602870
 DAKKS calibration certificate, humidity (device with permanently attached sensor); (test points: humidity 20 %, 50 %, 80 % and temperature approx. 23 °C)

further test points on request

CONDUCTIVITY

DAKKS-LF
 Item No. 605528
 DAKKS calibration certificate conductivity 3 test points, Test points 147 µS/cm, 1,413 µS/cm, 12.88 mS/cm

including 3 selectable points within
2 µS/cm - 1000 µS/cm

including 3 selectable points within
1 mS/cm - 150 mS/cm

every further test point
other measuring ranges on request